



PEG 400

Application note # QAN-0009 revA

PARAMETERS


NQAD
GAS: Air
FILTER: 1.3
GAIN: 10x
EVAPORATION TEMP: 35°C

HPLC
MOBILE PHASE:

Time (min)	ACN (%)	99% Water 1% ACN (%)
0	10	90
15.0	30	70
15.1	10	90
18.0	10	90

FLOW RATE: 1.0 mL/min
COLUMN: Alltima C18 5 um,
250 x 4.6 mm Alltech
COLUMN TEMP: Ambient
INJECTION VOLUME :5 µL

CHROMATOGRAM

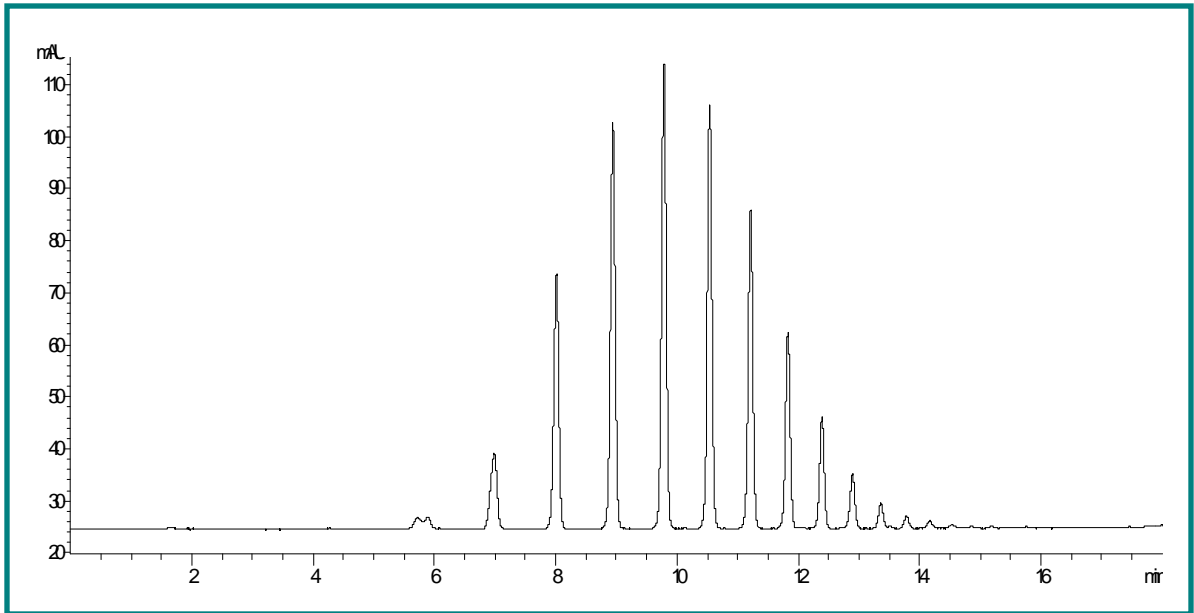

QUANT TECHNOLOGIES, LLC
1463 94TH Lane NE
Blaine, MN, USA 55449
763-398-0508
www.Quant-NQAD.com