



DIPHENHYDRAMINE LOD

Application note # QAN-0038

CHROMATOGRAMS


PARAMETERS

NQAD

GAS: Air
FILTER: 5 sec
GAIN: 50x
EVAPORATION TEMP: 35C

HPLC

MOBILE PHASE: 50:50 0.2% TFA in water: 0.2% TFA in ACN
FLOW RATE: 1.2 mL/min
COLUMN: Alltech Alltima HP C18, 3 u, 33 x 7.0 mm
COLUMN TEMP: Ambient
INJECTION VOLUME :10 uL
ANALYTE: Diphenhydramine

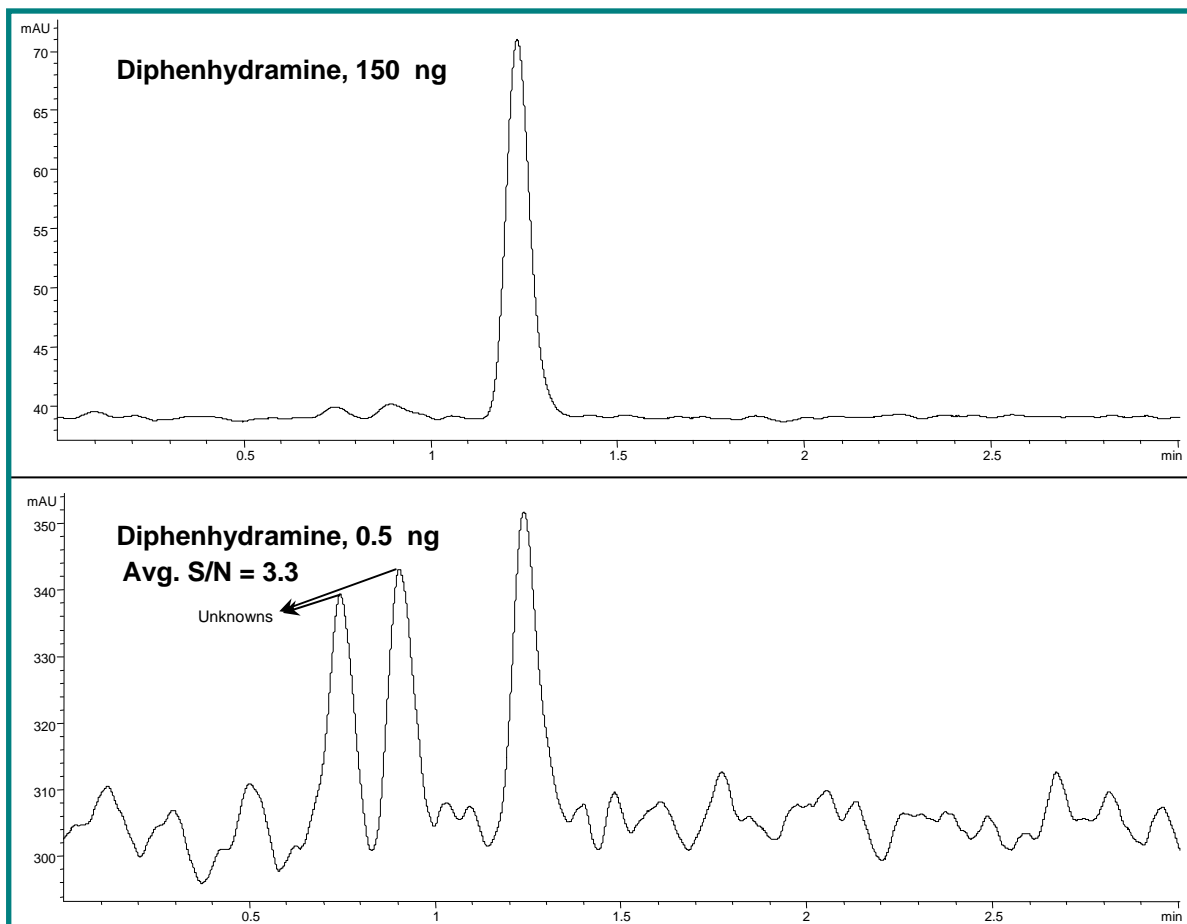

QUANT TECHNOLOGIES, LLC
1463 94TH Lane NE
Blaine, MN, USA 55449
763-398-0508
www.Quant-NQAD.com