



TWEEN 20

Application note # QAN-0039

PARAMETERS


NQAD

GAS: Air
FILTER: 5
GAIN: 10x
EVAPORATION TEMP: 35°C

HPLC

MOBILE PHASE: 30:70
methanol:water
FLOW RATE: 0.5 mL/min
COLUMN: Alltima C18, 3 μ M, 100 x
4.6 mm
COLUMN TEMP: Ambient
INJECTION VOLUME :10 μ L
ANALYTE: TWEEN 20, 1:50 (V/V)

CHROMATOGRAM

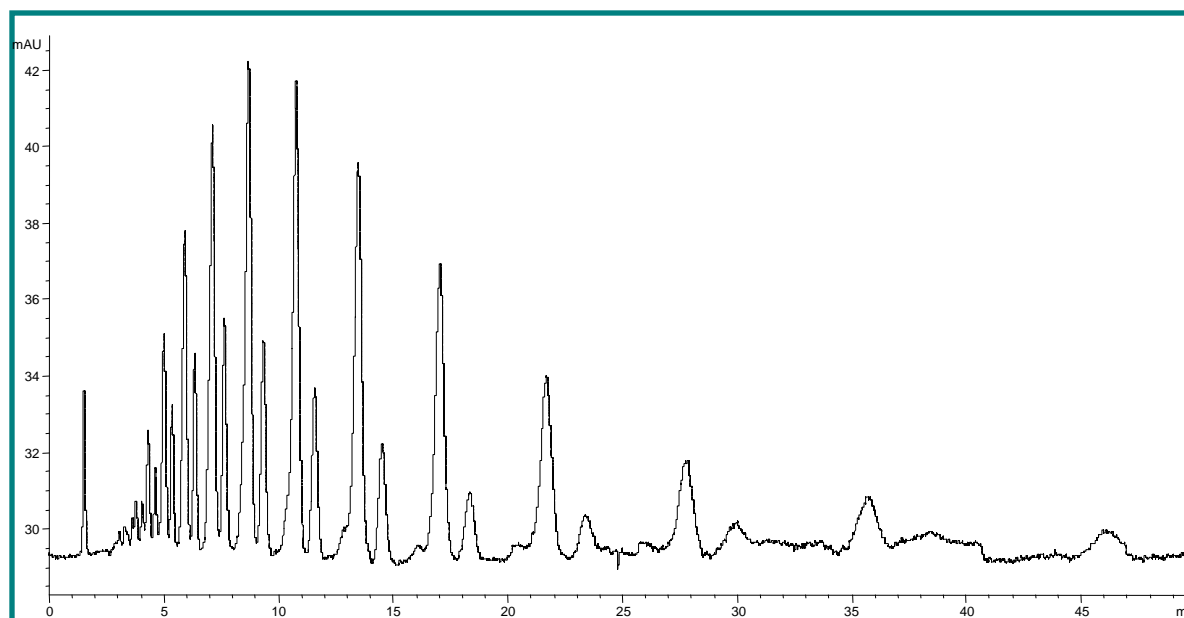

QUANT TECHNOLOGIES, LLC
1463 94TH Lane NE
Blaine, MN, USA 55449
763-398-0508
www.Quant-NQAD.com