



UREA REPRODUCIBILITY


Application note # QAN-0044

PARAMETERS

NQAD
GAS: Air
FILTER: 5 sec
GAIN: 1x
EVAPORATION TEMP: 35°C

HPLC
MOBILE PHASE: 40:60 Water:ACN
FLOW RATE: 1.0 mL/min
COLUMN: Alltech Alltima C18, 3u,
4.6 x 33 mm
COLUMN TEMP: Ambient
INJECTION VOLUME :10 µL
CONCENTRATION: 10,000 ng on
column
ANALYTE: Urea

CHROMATOGRAMS

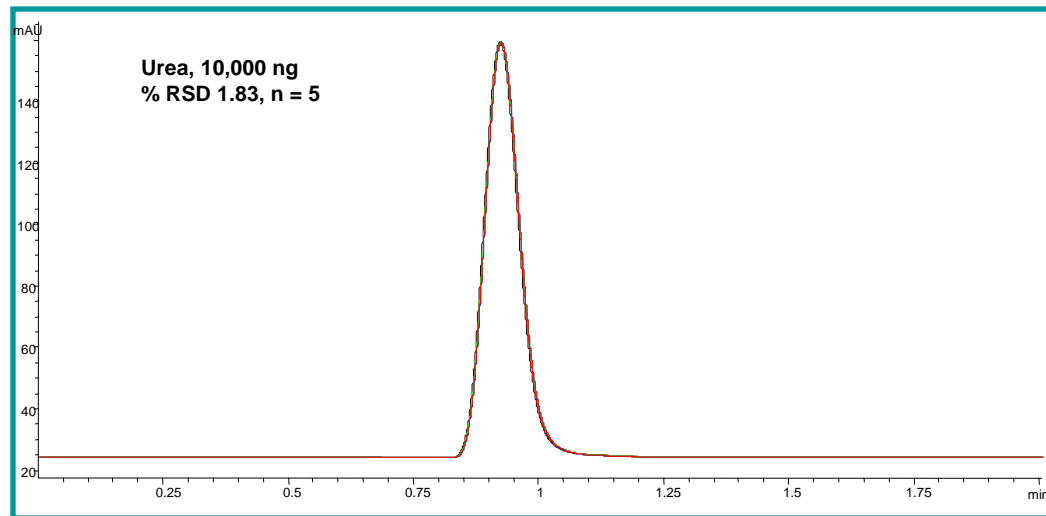

**QUANT TECHNOLOGIES,
LLC**
1463 94TH Lane NE
Blaine, MN, USA 55449
763-398-0508
www.Quant-NQAD.com