



PEG1000

Application note # QAN-0056

PARAMETERS

NQAD

GAS: Air
FILTER: 0.3 sec
GAIN: 10X
EVAPORATION TEMP: 35C


HPLC

MOBILE PHASE:

Time	Water	ACN
0	95	5
5	85	15
60	70	30

COLUMN: Agilent Eclipse Plus C18 5 μ , 150 x 4.6 mm
FLOW RATE: 1.2 mL/min
COLUMN TEMP: Ambient
INJECTION VOLUME : 1 μ L
CONCENTRATION: 1:100 (W:V)

CHROMATOGRAM

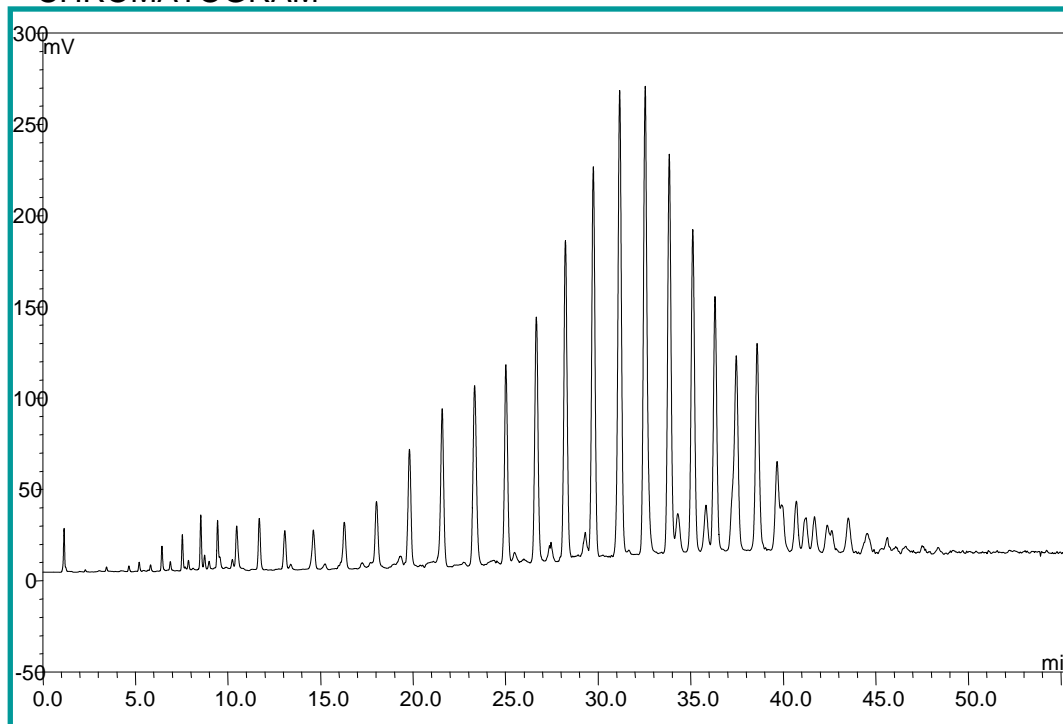

**QUANT TECHNOLOGIES,
LLC**
1463 94TH Lane NE
Blaine, MN, USA 55449
763-398-0508
www.Quant-NQAD.com